
MiniONE Button

Low Profile Balloon Gastrostomy Tube LEGACY + ENFIT®

Replacing AMT MiniONE® Balloon Button®

To ensure a proper fit, it is crucial to measure the stoma length using the AMT Balloon Stoma Measuring Device (BSMD). This is not a substitute for the DFU/IFU (Directions for Use/Instructions for Use).




DEFLATE BALLOON

Deflate the existing device using a Luer syringe or Luer Lock syringe.



REMOVE DEVICE

Remove the device, gently pull up on the device with slow and steady pressure.




PREPARE KIT

Prepare the new device, apply a water soluble lubricant to the device.



INSERT DEVICE

Insert the device into the stoma site, until it is flush against the skin. Remove the blue stiffener.




FILL BALLOON

Fill the balloon to the recommended fill volume, which is printed on the balloon fill valve.


Attaching an AMT Feed Set

The MiniONE® Balloon Button and corresponding feed set feature our patented Glow Green™ Technology.




STABILIZE

Stabilize the MiniONE® device.




ALIGN + INSERT

Align the marking lines and insert the connector into the MiniONE®.



ROTATE

Rotate connector 3/4 to the right.



LOCK

Lock the connector into place, now the device is ready to begin feeding.

Legacy + ENFit®


Available MiniONE® Balloon Button Sizes: 12F - 24F



MiniONE® also available in Non-Balloon Options:

MiniONE® Capsule Non-Balloon: 14F, 18F, 20F, 24F MiniONE® Non-Balloon: 14F, 18F, 20F, 24F

Feed Sets Included in Kit

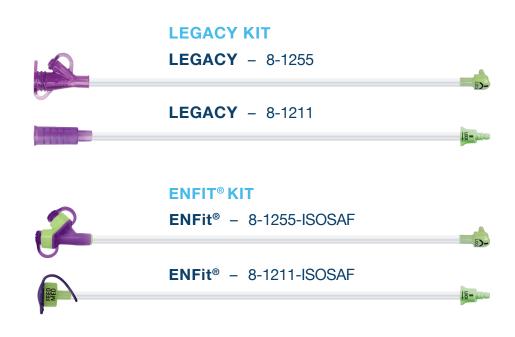

Questions? Call Today:

Jälleenmyyjä:

MEDI PLAST

Mediplast Fenno Oy PL 153, 01531 Vantaa Puh: 09 276 360

asiakaspalvelu@mediplast.com www.mediplast.com









For a complete list of products visit us at www.AppliedMedical.net 800 869 7382 | CS@AppliedMedical.net | ICS@AppliedMedical.net

